

# **Laser Sensor Development for Fluorescence Detection of Plastics and other Anthropogenic Compounds Dissolved in Seawater**

Dr. Paula G. Coble  
Department of Marine Science  
University of South Florida  
140 Seventh Ave. South  
St. Petersburg, FL 33701

Phone: (727)553-1631 Fax: (727)553-1189 Email: [pcoble@marine.usf.edu](mailto:pcoble@marine.usf.edu)

Dr. Dennis Killinger  
Physics Department  
University of South Florida  
Fowler Ave. Tampa, FL

Phone: (727)974-3995 Fax: (727)974-2635 Email: [killinge@chuma.cas.usf.edu](mailto:killinge@chuma.cas.usf.edu)

Grant #: N00014-96-1-5010

[http://www.onr.navy.mil/sci\\_tech/ocean/onrpgahm.htm](http://www.onr.navy.mil/sci_tech/ocean/onrpgahm.htm)

## **LONG TERM GOALS**

The long-term goal is to build and deploy a highly sensitive, *in situ* AUV-mounted instrument optimized for distinguishing natural colored dissolved organic matter (CDOM) in seawater as well as locating and identifying plastic and rubber-coated objects, such as mines, in the water column and buried within the seafloor. Oceanographic applications include UV-vis spectral characterization of dissolved and particulate (phytoplankton) fluorescence for remote sensing, plume tracking, and pollution applications. The multi-channel UV laser-induced fluorescence sensor (MUVLIFS) will ultimately be integrated and deployed on an autonomous underwater vehicle (AUV) to enhance strategic and oceanographic applications.

## **OBJECTIVES**

The short-term goal is to improve the design for a compact UV laser multi-channel fluorometer system for shipboard use in enhanced measurement of UV-stimulated fluorescent compounds in seawater. During the past year, we have developed a compact, multi-laser LIF (laser induced fluorescence) system with optical filtered PMT detector that provides increased sensitivity by several orders of magnitude over existing *in situ* instrumentation.

## **APPROACH**

During this funding year the LIF system was modified to enhance the detection of CDOM in natural waters, including doubling the number of fluorescence emission channels at selected CDOM wavelengths, adding another laser excitation wavelength, and adding laser (optical path) absorption measurements. The control electronics were enhanced, reduced in size for portability, and extensive automated software was developed to permit automated data collection and real-time display. The new multi-laser induced fluorescence (LIF) system was tested successfully on a five day extended cruise

Report Documentation Page			Form Approved OMB No. 0704-0188		
Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.					
1. REPORT DATE <b>30 SEP 2003</b>		2. REPORT TYPE		3. DATES COVERED <b>00-00-2003 to 00-00-2003</b>	
4. TITLE AND SUBTITLE <b>Laser Sensor Development for Fluorescence Detection of Plastics and other Anthropogenic Compounds Dissolved in Seawater</b>			5a. CONTRACT NUMBER		
			5b. GRANT NUMBER		
			5c. PROGRAM ELEMENT NUMBER		
6. AUTHOR(S)			5d. PROJECT NUMBER		
			5e. TASK NUMBER		
			5f. WORK UNIT NUMBER		
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) <b>Department of Marine Science,,University of South Florida,140 Seventh Ave. South,,St. Petersburg,FL,33701</b>			8. PERFORMING ORGANIZATION REPORT NUMBER		
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)			10. SPONSOR/MONITOR'S ACRONYM(S)		
			11. SPONSOR/MONITOR'S REPORT NUMBER(S)		
12. DISTRIBUTION/AVAILABILITY STATEMENT <b>Approved for public release; distribution unlimited</b>					
13. SUPPLEMENTARY NOTES					
14. ABSTRACT <b>The long-term goal is to build and deploy a highly sensitive, in situ AUV-mounted instrument optimized for distinguishing natural colored dissolved organic matter (CDOM) in seawater as well as locating and identifying plastic and rubber-coated objects, such as mines, in the water column and buried within the seafloor. Oceanographic applications include UV-vis spectral characterization of dissolved and particulate (phytoplankton) fluorescence for remote sensing, plume tracking, and pollution applications. The multi-channel UV laser-induced fluorescence sensor (MUVLIFS) will ultimately be integrated and deployed on an autonomous underwater vehicle (AUV) to enhance strategic and oceanographic applications.</b>					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT <b>Same as Report (SAR)</b>	18. NUMBER OF PAGES <b>7</b>	19a. NAME OF RESPONSIBLE PERSON
a. REPORT <b>unclassified</b>	b. ABSTRACT <b>unclassified</b>	c. THIS PAGE <b>unclassified</b>			


into the Gulf of Mexico in which a variety of water masses were sampled to determine instrument sensitivity under environmental conditions. In addition, a cruise off the coast of Australia was also made, but this was not as successful due to equipment damage going through customs/shipment. This system serves as the prototype for the *in situ* MUVLIFS sensor.

## WORK COMPLETED


Previous work (1996-2001) reported the laboratory tests of three different LIF prototype configurations. The most sensitive and portable of the prototypes consisted of a microchip laser (5 mW) at 266 nm, a PMT detector and 5 optical filter channels, and improved upon the sensitivity of current *in situ* fluorometers by a factor of 100 to 0.01 ppb of quinine sulfate.

During the previous year (FY02), this configuration was further modified to include more spectral band filters allowing for greater fluorescence characterization of environmental samples. The current portable system uses a (4x) Nd:YAG microchip laser source operating at 266 nm and thirteen (spectral-band filter) detection channels monitoring scatter and fluorescence: 239 nm, 266 nm (Rayleigh), 289 nm (Raman), 301 nm, 314 nm, 334 nm, 370nm, 400 nm, 420 nm, 436 nm, 451 nm, 470 nm and 685 nm. Absorption filters were installed with cutoff at 285 nm and 295 nm, with a PMT detector and a boxcar integrator averaging system. A laptop computer is used via GPIB interface for data acquisition and controlling the filter wheel. The collection system has been improved by using multi-pass geometry of the laser beam through the cell, and adding a spherical mirror at the back of the flow cell along the collection axis. The multi-pass and spherical mirror configuration of the optical system show 67% increase in signal at the 450 nm optical channel over single-pass configurations. The detection limit of the modified portable system is 0.001 ppb of quinine sulfate. This is 10 times more sensitive than originally predicted, and 1000 times more sensitive than current multichannel *in situ* fluorometers. It should be noted that the increased sensitivity of this LIF configuration is due to the use of a high PRF (Pulse Repetition Frequency) laser that operates at a 8 KHz pulse rate, the use of a high speed box car integrator that can detect and average the individual fluorescence pulses at 8 KHz, and the use of a PMT for increased light sensitivity.

During the past year (FY03), 11 additional filter wavelength channels (and an additional filter wheel) have been added to permit greater spectral resolution. New software programs were written in Labview to acquire, store and monitor the optical channels in real-time. The emission channels can be switched every few seconds, resulting in a complete scan in about one minute. In addition, another excitation laser at a different wavelength (355 nm) has been added so that different fluorescence signatures can be measured. Also, the optical layout of the system was changed to permit direct absorption (transmission) measurements of the water samples for both the 266 nm and the 355 nm wavelengths. Figure 1 shows a schematic of the two wavelength portable LIF system. Figure 2a shows the portable system in two sealed cases: case 1 contained the boxcar, filter wheel electronics and case 2 contained the laser source, filter wheel, PMT, and the optical collection system (Figure 2b).

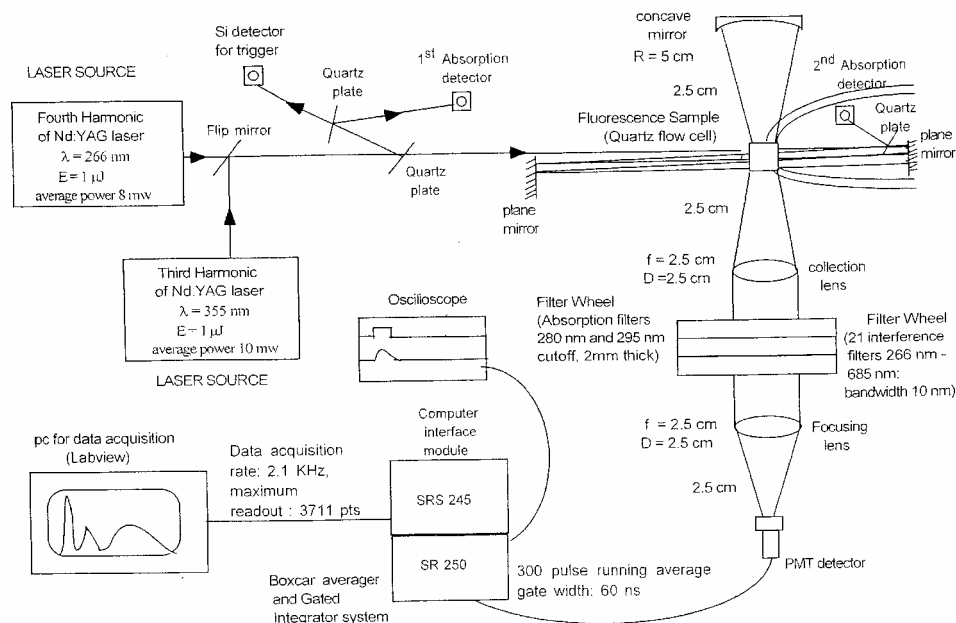

**Figure 1. Schematic of the equipment setup of the portable Laser Induced Fluorescence (LIF) system**

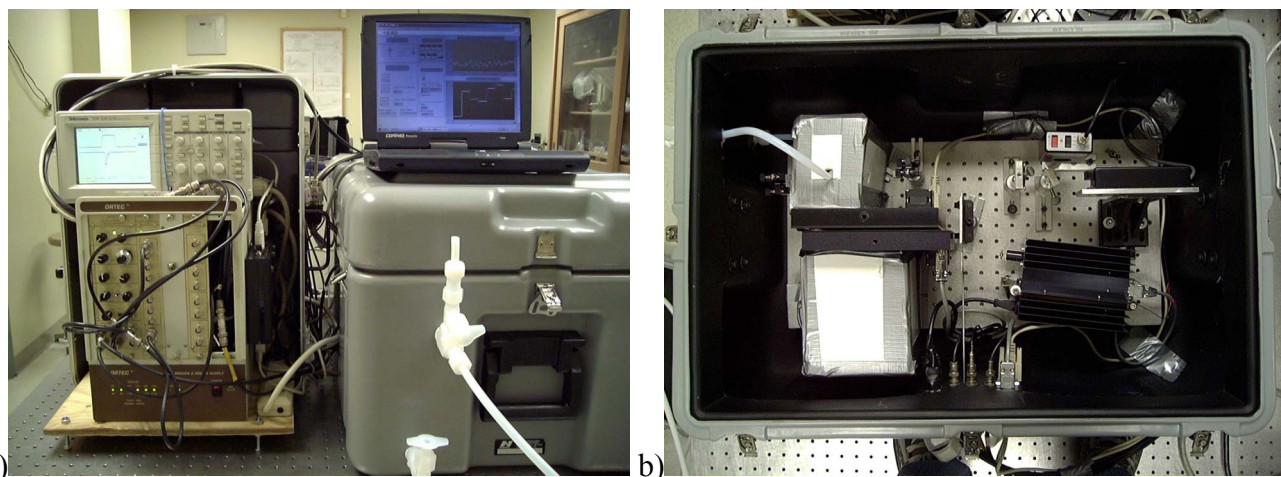

**Figure 2a. Picture of the portable laser induced fluorescence system; b. Picture of the optical system for the portable LIF showing laser source, filter wheel and PMT detector**


## RESULTS

The modified LIF prototype was tested on a 5 day cruise (RV Suncoaster; May 16-21, 2003) to determine instrument sensitivity in a variety of water masses using the ships underway water supply. The cruise track was in the Gulf of Mexico from Kew West to Tampa Bay which also included clean water masses, up-river samples, and DOC plume detection. In addition to the portable LIF system, a commercially available multi-channel *in situ* fluorometer was also used to monitor real-time CDOM fluorescence from the underway water system. The SAFire (Wetlabs; Philomath, OR, USA) represents

the state of the art for *in situ* fluorometers. Its estimated sensitivity is 1 ppb of quinine sulfate, and its multiple excitation and emission channels make it unique in the market.

Discrete water samples taken from the underway system for comparison were analyzed by excitation emission matrix (EEM) spectroscopy on a FluoroMax-2 (JY-SPEX; Princeton, NJ, USA). EEM spectroscopy samples were filtered (0.7 micron GFF), corrected for instrument variability, blank subtracted and normalized to quinine sulfate equivalents (Coble, 1996).

We are now analyzing the data and expect to be able to report on the sensitive LIF measurements shortly. Of importance is the fact that the system also provided real-time fluorescence and absorption data so that an estimate of the DOC signal and water composition could be made as the cruise progressed. Figure 3 shows an example of the real-time data during the 5-day Gulf of Mexico cruise.

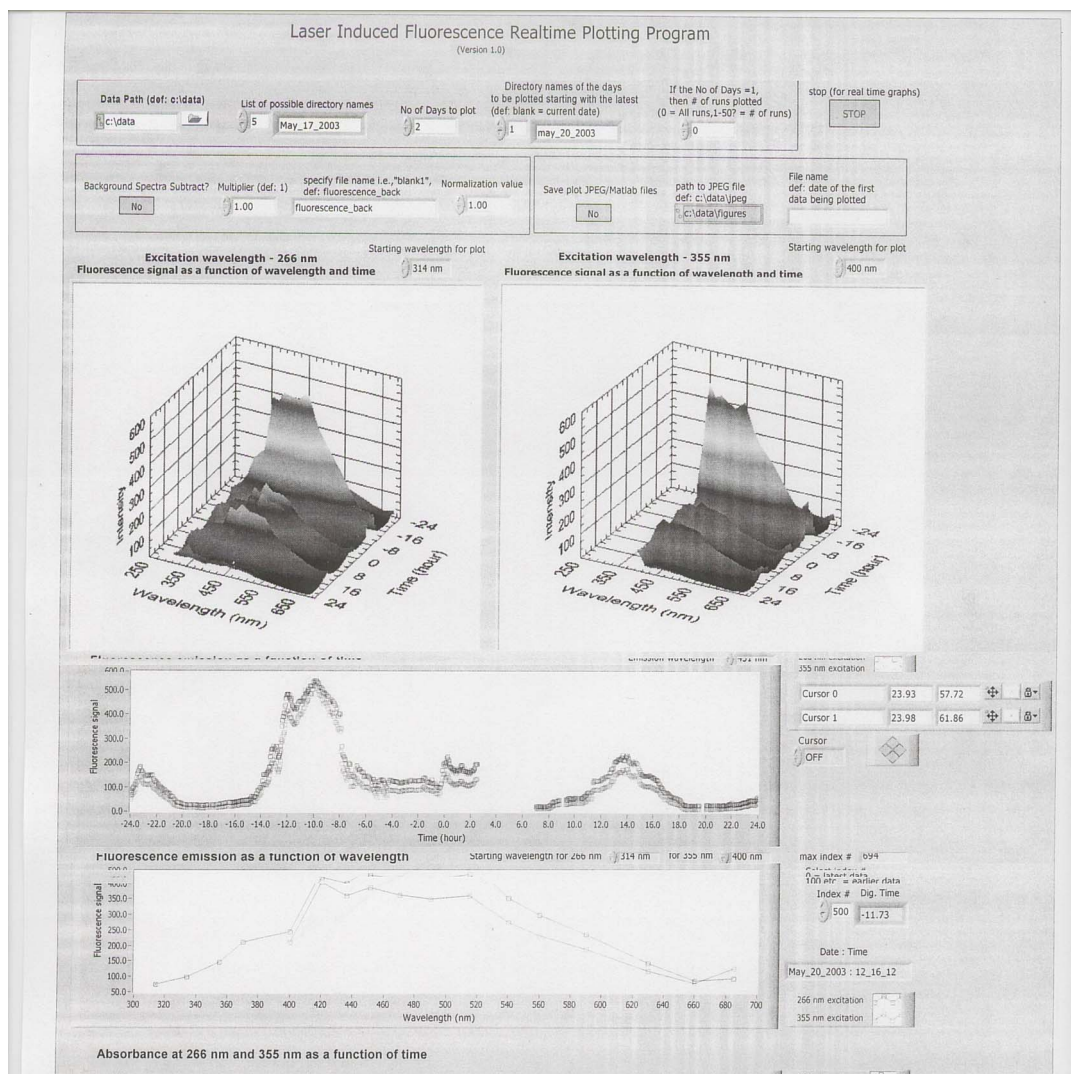

**Figure 3: Image of computer screen showing real-time and time-history plot of fluorescence signal, absorption signal, and individual fluorescence channel**

## IMPACT/APPLICATIONS

Development of a compact, *in situ*, UV multi-channel LIF sensor is at the cutting edge of scientific and technological development. Applications range from study of trace constituents in the atmosphere to tracking pollutants in natural waters. Miniaturization, multi-channel spectral capability, low detection limits and extension of detection into the UV are features now being rapidly advanced. As with most past examples of instrument development, the full range of applications and their value to science, defense, industry and society have yet to be fully explored.

## RELATED PROJECTS

The MUVLIFS unit is targeted for multisensor applications to increase the level of certainty that a mine does or does not exist. We will test the performance of both shipboard and AUV systems in local waters in conjunction with an ongoing study. We will assess sensor performance for oceanographic applications.

## PUBLICATIONS

Del Castillo, C.E., P.G. Coble, R.N. Conmy, F.E. Muller-Karger, L. Vanderbloomen, and G.A. Vargo. 2001. Multispectral In-situ Measurements of Organic Matter and Chlorophyll Fluorescence in Seawater: Documenting the Intrusion of the Mississippi River Plume in the West Florida Shelf (in press: Limnology and Oceanography)

Richards. 2001. Laser Induced Fluorescence Signal to Noise Measurements using Optical Fiber Coupled PMT Detectors. Master Thesis, Dept. of Physics, University of South Florida, Tampa, Florida.

Boehme, J. R. Artificial and natural fluorescence of dissolved organic matter in the Tampa Bay Estuary. Ph.D. Dissertation, University of South Florida, 2000.

Boehme, J. R. and Coble, P.G. 2000. Characterization of dissolved organic matter using high energy laser fragmentation. Environmental Science and Technology, 34(15) 3283-3290.

Sivaprakasam, V. 1999. Geometrical and Polarization effects on Laser Induced Raman Scatter and Fluorescence Emission of Quinine Sulfate and Trace Species in Water. Master Thesis, Dept. of Physics, University of South Florida, Tampa, Florida

Sivaprakasam, Vasanthi. 2002. UV Laser Induced Fluorescence Spectroscopic studies and Trace detection of dissolved plastics (Bisphenol-A) and Organic Compounds in Water. Ph.D. Dissertation, Department of Physics, University of South Florida, 2002

Sivaprakasam, Vasanth and Killinger, D.K. 2003. Effect of polarization and geometrical factors on quantitative laser induced fluorescence to Raman intensity ratios of water samples and a new calibration technique, J. Opt. Soc. Am. B 20, 1980-1989 .

Sivaprakasam, Vasanthi and Killinger, D.K. 2003. Tunable UV Laser induced Fluorescence detection of trace plastics and Dissolved Organic Compounds (DOC) in water, Accepted for publication, Applied Optics, 2003.

Sivaprakasam, Vasanthi, Shannon, Robert F. Jr., Luo, Caiyan, Coble, Paula. G., Boehme, Jennifer R. and Killinger, Dennis K. 2003. Development and initial calibration of a portable Laser Induced Fluorescence system used for in situ measurements of trace plastics and Dissolved Organic Compounds in seawater and the Gulf of Mexico, Accepted for publication, Applied Optics, 2003.

Timperman, A.T., and Paula G. Coble. 1998. Analysis of proteins and peptides in seawater using capillary electrophoresis. Journal of Chromatography A, 829: 309-315.

Nase, V. 1998. Dependence of CCD Signal-To-Noise Values on Optical Excitation and Collection Geometry in Laser Induced Fluorescence, Master Thesis, Dept. of Physics, University of South Florida, Tampa, Florida.

Bengtsson, M., and L.-G. Nilsson. 1996. Development and evaluation of a laser-induced fluorescence experiment for the detection of trace compounds in water using a tunable UV-OPO system. Master Thesis, Lund University, Lund, Sweden.